



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaca Holland/Jan van den Hoek
Rijksstraatweg 94
Numansdorp 3281LW Netherlands

Date: 06/03/1

Test No: 47767


Animal and Sample Description

Animal Name: AH Peruvian Grandstander
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 0007024F80
Sample Location: Side
Sample Date: 04/23/14
Age: 07/10/13

Laboratory Data

Mean Fiber Diameter:	19.6 microns	Fibers Greater Than 30 microns:	0.7 %
Standard Deviation:	3.4 microns	Comfort Factor:	99.3 %
Coefficient of Variation:	17.1 %	Mean Curvature:	39.3 deg/mm
Spin Fineness:	18.5 microns	SD Curvature:	21.0 deg/mm

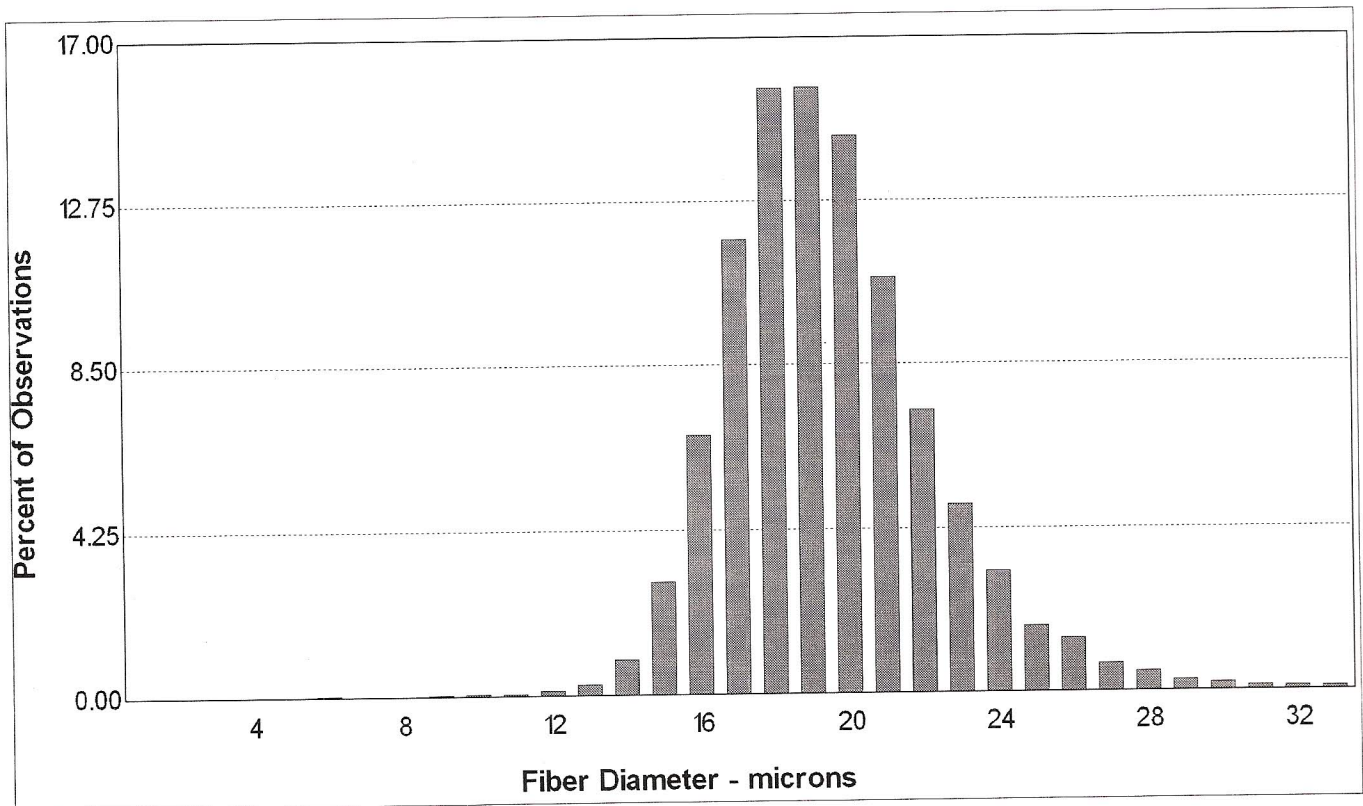

This Test Performed According to I.W.T.O Method 47