

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Alpaca Holland/Jan van den Hoek  
Rijksstraatweg 94  
Numansdorp 3281 LW Holland

08/24/11

Test No: 416285


### Animal and Sample Description

**Animal Name:** AH Peruvian Huascar Inca  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Fawn

**Animal ID:** 0006E94272  
**Sample Location:** Side  
**Sample Date:** 04/21/11  
**Age:** 07/28/09

### Laboratory Data

**Mean Fiber Diameter:** 19.3 microns  
**Standard Deviation:** 3.9 microns  
**Coefficient of Variation:** 20.0 %  
**Fibers Greater Than 30 microns:** 1.6 %

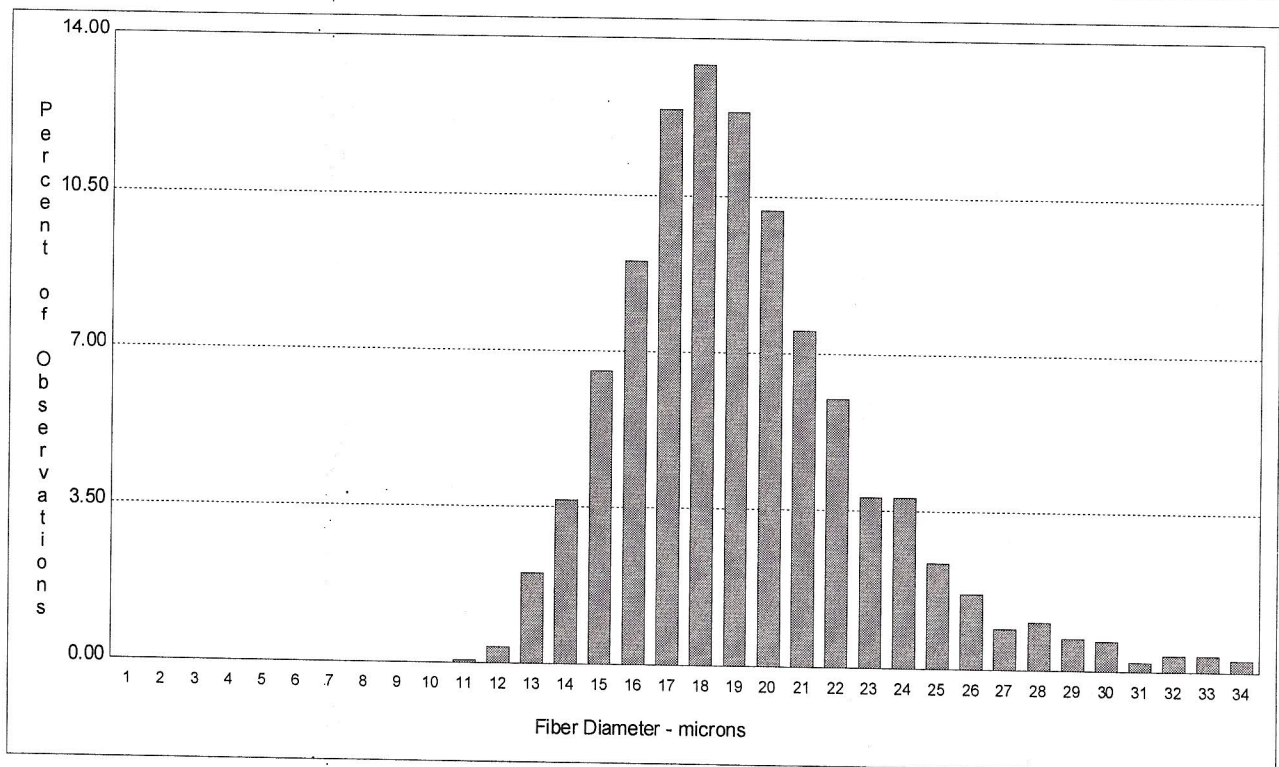

This Test Performed According to I.W.T.O Method 12