

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaka Zucht Verband Deutschland e.V./Attn: Mike Herrling
Upsteder Str. 31
Wittmund D-26409 Germany

Date: 03/27/08

Test No: 318225


Animal and Sample Description

Animal Name: AH Peruvian Cusco 00067097A7
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 2008-00655
Sample Location: L Flank
Sample Date: 03/01/08
Age: 06/01/06

Laboratory Data

Mean Fiber Diameter:	25.6 microns	Fibers Greater Than 30 microns:	11.1 %
Standard Deviation:	4.0 microns	Comfort Factor:	88.9 %
Coefficient of Variation:	15.4 %	Mean Curvature:	28.6 deg/mm
Spin Fineness:	23.9 microns	SD Curvature:	17.0 deg/mm

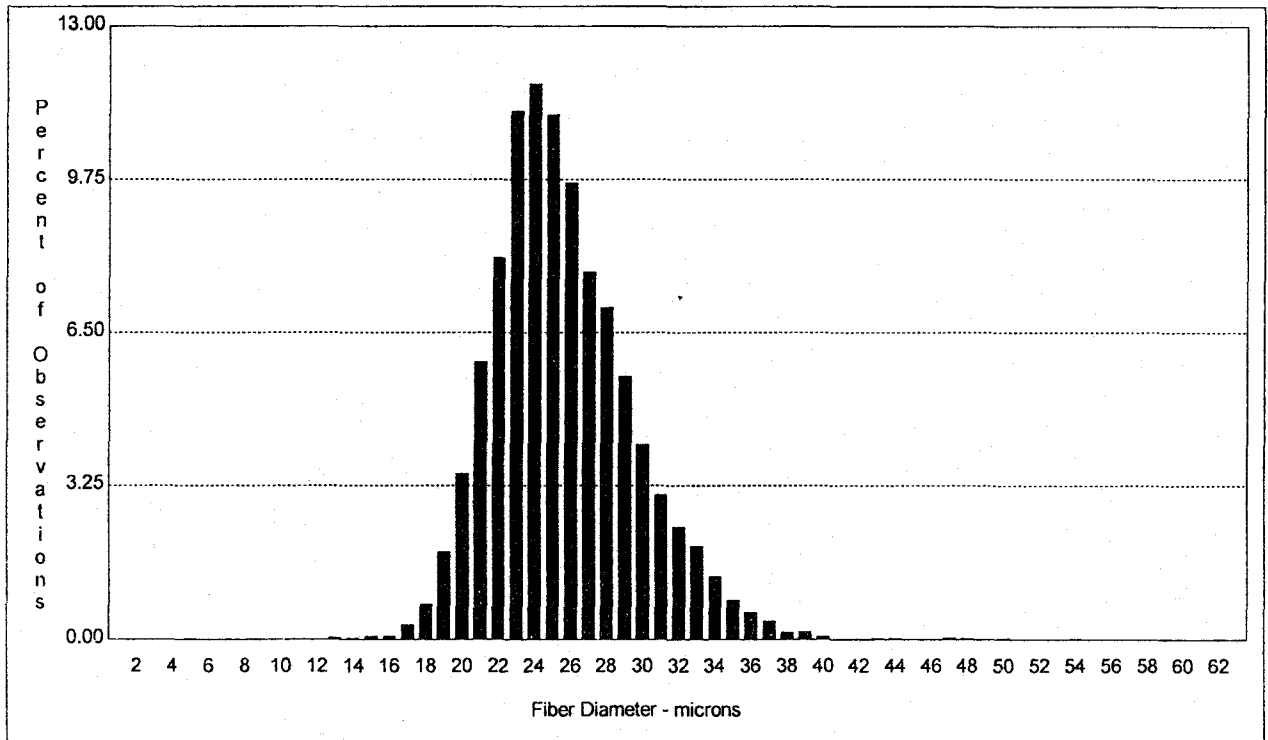

This Test Performed According to I.W.T.O Method 47