



## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaca Holland/Jan van den Hoek  
Rijksstraatweg 94  
Numansdorp 3281LW Netherlands

Date: 05/14/15

Test No: 500948


#### Animal and Sample Description

**Animal Name:** AH Peruvian Grandstander  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White

**Animal ID:** 7024F80  
**Sample Location:** Side  
**Sample Date:** 04/17/15  
**Age:** 07/10/13

#### Laboratory Data

<b>Mean Fiber Diameter:</b>	18.0 microns	<b>Fibers Greater Than 30 microns:</b>	0.6 %
<b>Standard Deviation:</b>	3.3 microns	<b>Comfort Factor:</b>	99.4 %
<b>Coefficient of Variation:</b>	18.5 %	<b>Mean Curvature:</b>	46.3 deg/mm
<b>Spin Fineness:</b>	17.2 microns	<b>SD Curvature:</b>	24.4 deg/mm

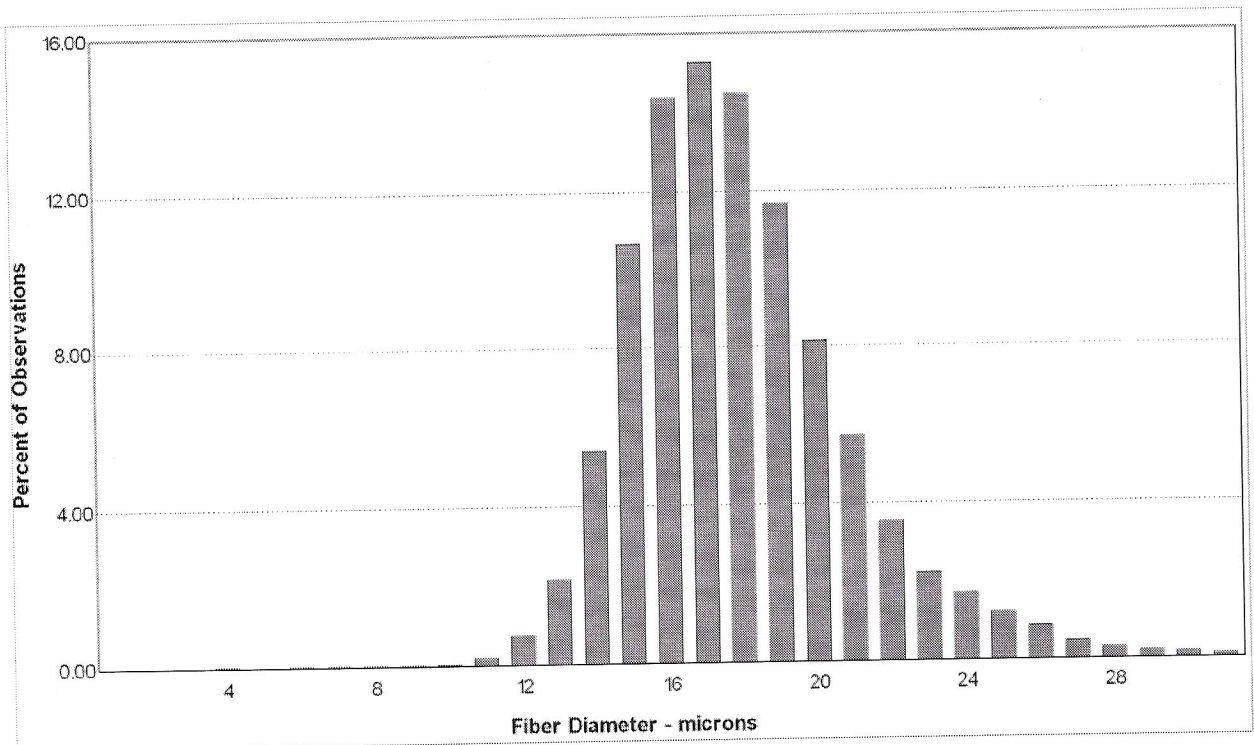

This Test Performed According to I.W.T.O Method 47