

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Alpaca Holland/Jan van den Hoek
Rijksstraatweg 94
Numansdorp 3281LW Netherlands

07/28/12

Test No: 436950


Animal and Sample Description

Animal Name: AH Peruvian Julian
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 0006E8A956
Sample Location: Side
Sample Date: 05/02/12
Age: 07/07/11

Laboratory Data

Mean Fiber Diameter:	15.9 microns	Spin Fineness:	15.0 microns
Standard Deviation:	2.8 microns	Mean Curvature (deg/mm):	50.5
Coefficient of Variation:	17.2 %	SD Curvature (deg/mm):	27.8
Fibers Greater Than 30 microns:	0.2 %	Comfort Factor:	99.8 %
Medullated Fibers:	3.5 %		

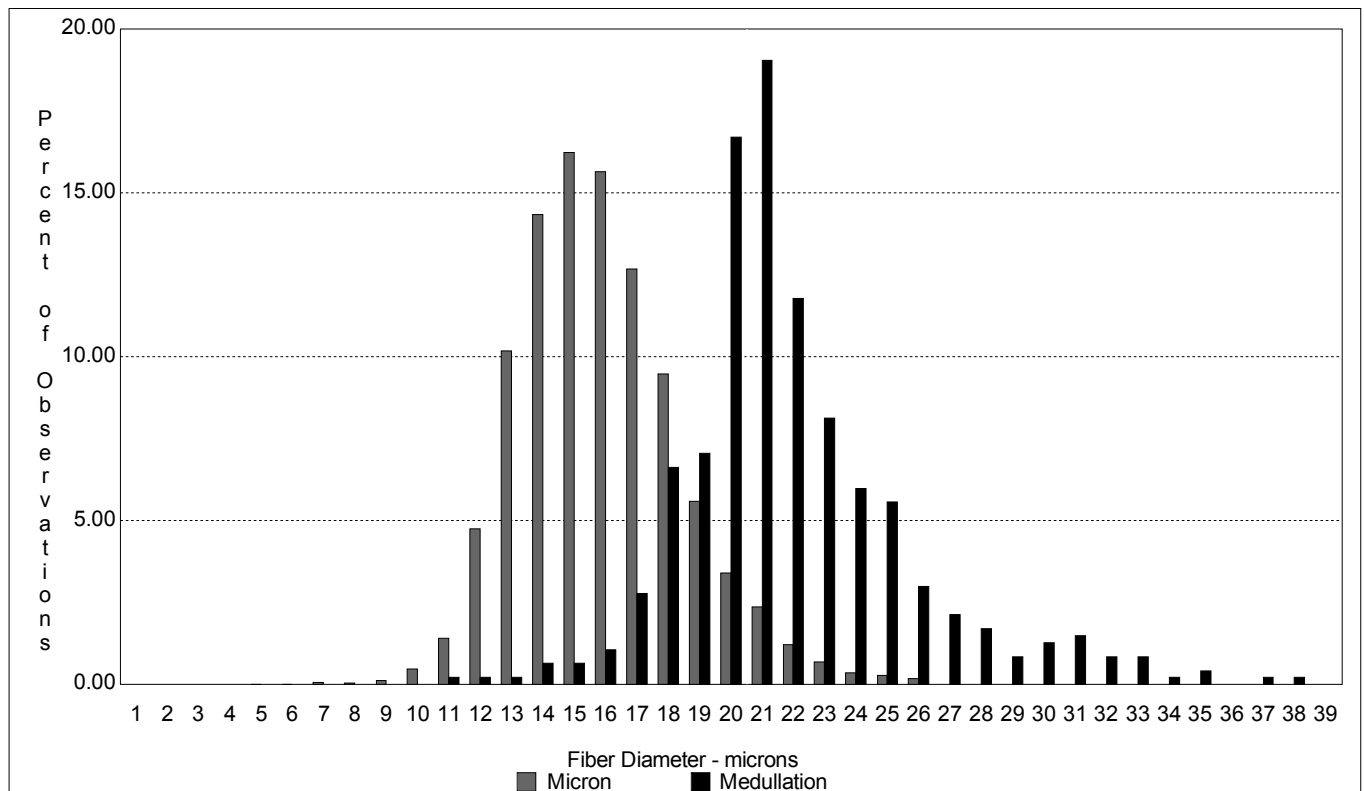

This Test Performed According to I.W.T.O Method 47