

**Yocom-McColl Testing Laboratories, Inc.**  
540 West Elk Place • Denver, Colorado 80216-1823 USA  
PHONE (303) 294-0582 • FAX (303) 295-6944  
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan  
Micron Test Report**

Alpaca Holland/Jan van den Hoek  
Rijksstraatweg 94  
Numansdorp 3281 LW Holland

08/24/11

**Test No:** 416290


**Animal and Sample Description**

**Animal Name:** AH Peruvian Valentino  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White

**Animal ID:** 0006736D5B  
**Sample Location:** Side  
**Sample Date:** 04/21/11  
**Age:** 07/17/08

**Laboratory Data**

**Mean Fiber Diameter:** 21.7 microns  
**Standard Deviation:** 4.3 microns  
**Coefficient of Variation:** 20.0 %  
**Fibers Greater Than 30 microns:** 3.5 %

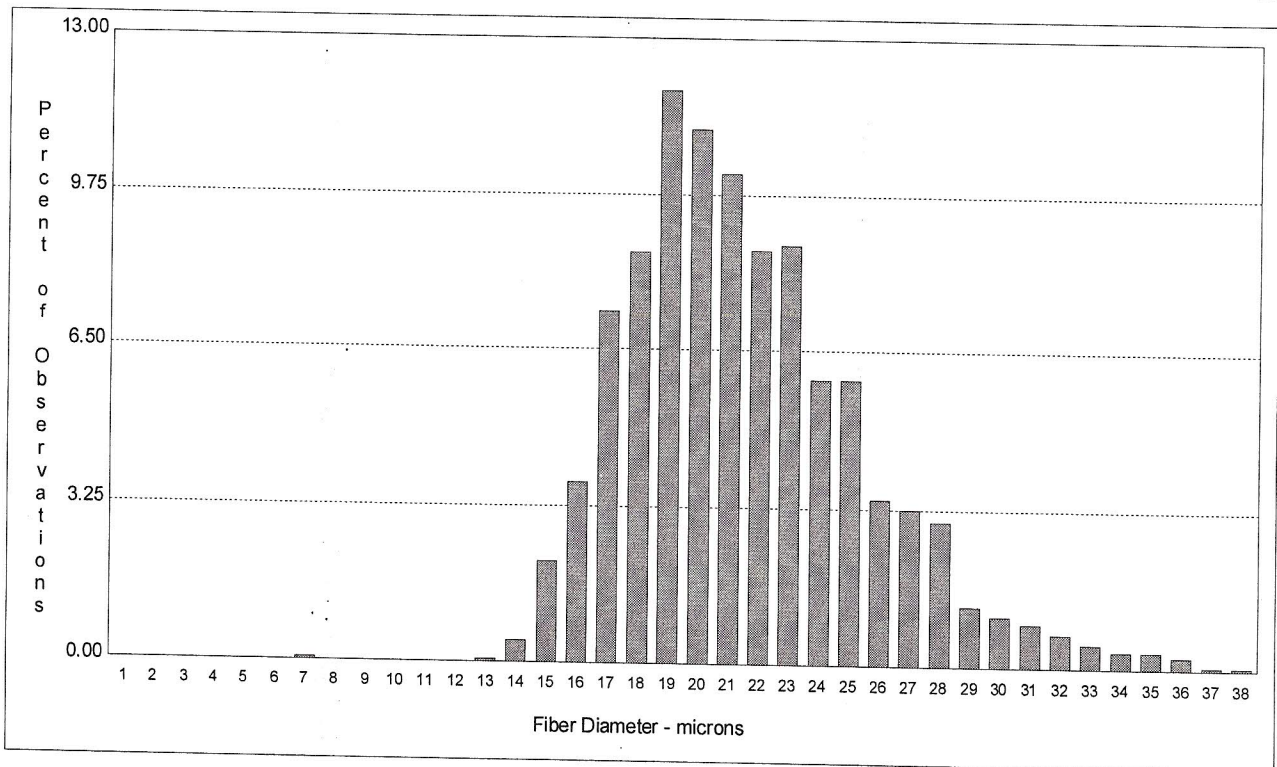

**This Test Performed According to I.W.T.O Method 12**