

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaka Zucht Verband Deutschland e.V./Attn: Mike Herring  
Upsteder Str. 31  
Wittmund D-26409 Germany

Date: 06/04/07

Test No: 295861


### Animal and Sample Description

Animal Name: AH Peruvian Casanova 528210000241099  
Breed: Alpaca(Huacaya)  
Sex: Male  
Color: Med Grey

Animal ID: 2007-00406  
Sample Location: L Flank  
Sample Date: 05/05/07  
Age: 06/01/02

### Laboratory Data

|                           |              |                                 |             |
|---------------------------|--------------|---------------------------------|-------------|
| Mean Fiber Diameter:      | 23.6 microns | Fibers Greater Than 30 microns: | 11.3 %      |
| Standard Deviation:       | 6.3 microns  | Comfort Factor:                 | 88.7 %      |
| Coefficient of Variation: | 26.8 %       | Mean Curvature:                 | 46.0 deg/mm |
| Spin Fineness:            | 24.3 microns | SD Curvature:                   | 26.8 deg/mm |

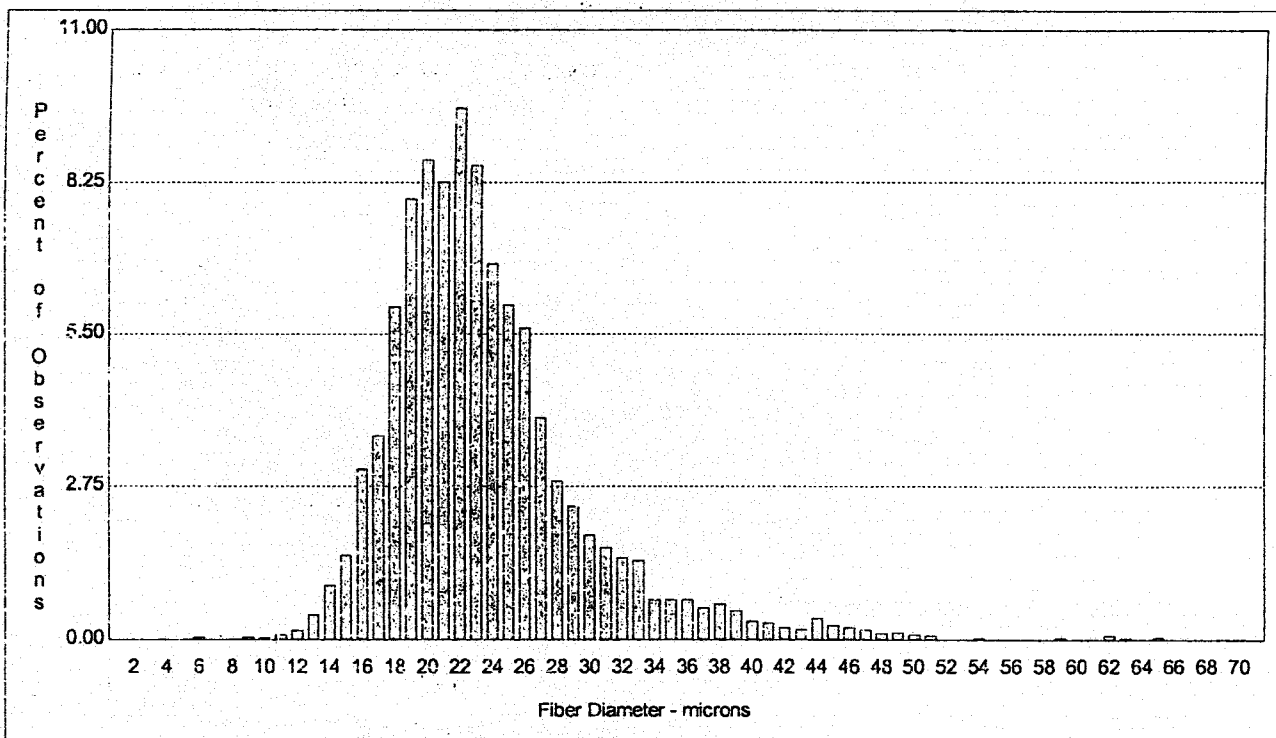

This Test Performed According to I.W.T.O Method 47