



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaka Zucht Verband Deutschland e.V./Attn: Mike Herring
Upsteder Str. 31
Wittmund D-26409 Germany

Date: 06/04/07

Test No: 295843


Animal and Sample Description

Julio
Animal Name: Peruvian Matador 982009105066562
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 2007-00410
Sample Location: L Flank
Sample Date: 05/05/07
Age: 05/01/06

Laboratory Data

Mean Fiber Diameter:	21.3 microns	Fibers Greater Than 30 microns:	2.4 %
Standard Deviation:	4.3 microns	Comfort Factor:	97.6 %
Coefficient of Variation:	20.3 %	Mean Curvature:	39.1 deg/mm
Spin Fineness:	20.6 microns	SD Curvature:	23.5 deg/mm

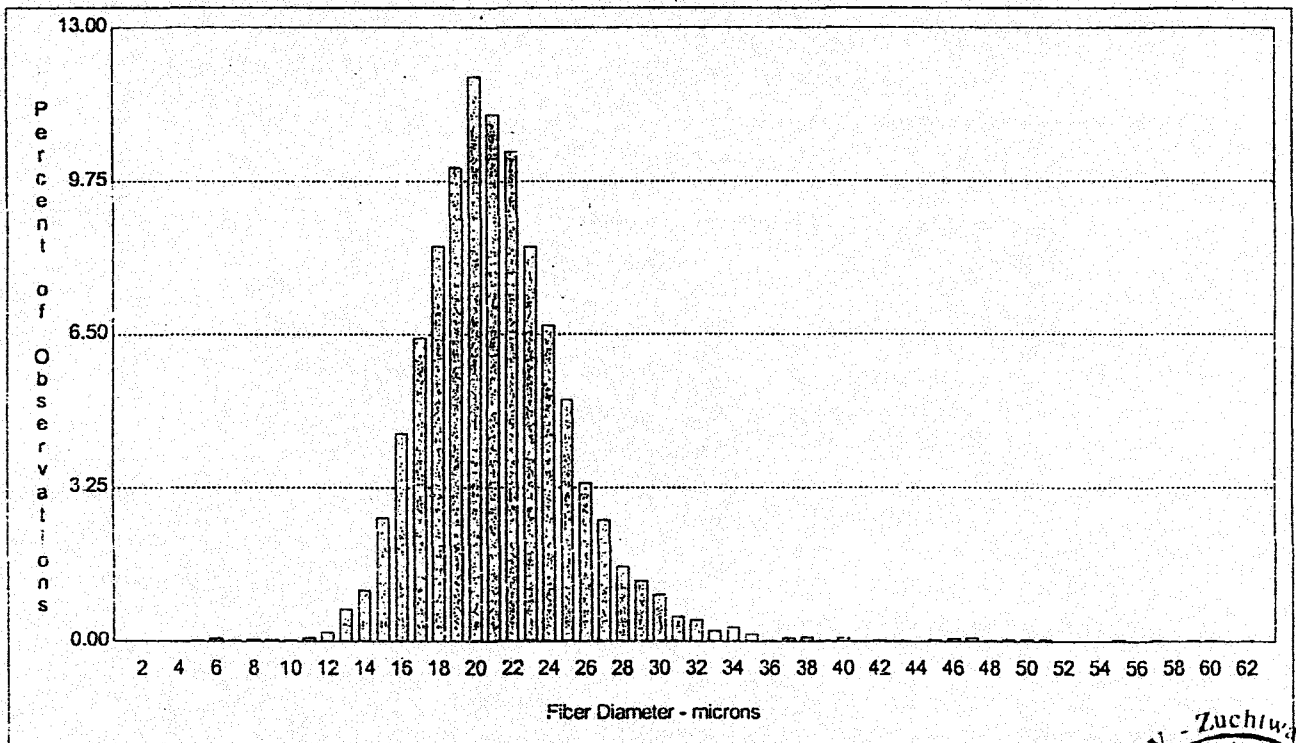

This Test Performed According to I.W.T.O Method 47

